

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01333	Calib. Date: 01/06/2010
Certification File No.:	01334	Calib. No.: 00010
Linearity File No.:	01335	Cert. Date: 01/06/2010
Solution File No.:	01409	Cert. No.: 00008
Sequential File No.:	01409	Lin. Date: 01/06/2010
		Lin. No.: 00008
		Soln. Date: 04/24/2010
		Soln. No.: 00123
		File Date: 04/24/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0340
Solution Control Lot:	09I069	Expires: 09/18/2011
		Bottle No.: 1383

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:32D		
Control 1 EC	0.101%	04:32D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	04:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:33D		
Control 2 EC	0.100%	04:33D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	04:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:34D		
Control 3 EC	0.100%	04:35D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	04:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:35D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____

[Handwritten Signature] 149

Badge No.: 149

Date: 04/24/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	01333	Calib. Date:	01/06/2010
Certification File No.:	01334	Cert. Date:	01/06/2010
Linearity File No.:	01335	Lin. Date:	01/06/2010
Solution File No.:	01414	Soln. Date:	05/02/2010
Sequential File No.:	01414	File Date:	05/02/2010
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0340
Solution Control Lot:	09I069	Expires:	09/18/2011
		Bottle No.:	0008

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:45D		
Control 1 EC	0.102%	02:46D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	02:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:47D		
Control 2 EC	0.101%	02:47D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	02:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:48D		
Control 3 EC	0.102%	02:49D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.102%	02:49D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:49D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MOLES

First Name: VITO

MI: M

Signature: _____

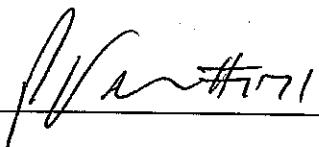

Badge No.: 171

Date: 05/02/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01333	Calib. Date: 01/06/2010
Certification File No.:	01334	Cert. No.: 00010
Linearity File No.:	01335	Cert. Date: 01/06/2010
Solution File No.:	01428	Lin. No.: 00008
Sequential File No.:	01428	Soln. Date: 05/28/2010
		Soln. No.: 00125
		File Date: 05/28/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0340
Solution Control Lot:	09I069	Expires: 09/18/2011
		Bottle No.: 0016

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:18D		
Control 1 EC	0.100%	13:19D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:20D		
Control 2 EC	0.100%	13:20D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:21D		
Control 3 EC	0.100%	13:21D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:22D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature:



Badge No.: 127

Date: 05/28/2010

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C		Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.		
Calibration File No.: 01333	Calib. Date: 01/06/2010	Calib. No.: 00010
Certification File No.: 01334	Cert. Date: 01/06/2010	Cert. No.: 00008
Linearity File No.: 01335	Lin. Date: 01/06/2010	Lin. No.: 00008
Solution File No.: 01442	Soln. Date: 06/20/2010	Soln. No.: 00126
Sequential File No.: 01442	File Date: 06/20/2010	

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUN S3-0340
Control Solution %: 0.100%		Expires: 09/18/2011
Solution Control Lot: 09I069		Bottle No.: 0021

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:52D		
Control 1 EC	0.100%	18:53D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	18:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:53D		
Control 2 EC	0.099%	18:54D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	18:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:55D		
Control 3 EC	0.099%	18:55D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	18:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:56D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MOLES

First Name: VITO

MI: M

Signature: _____



Badge No.: 171

Date: 06/20/2010

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01460 Calib. Date: 07/06/2010 Calib. No.: 00011
Certification File No.: 01461 Cert. Date: 07/06/2010 Cert. No.: 00009
Linearity File No.: 01462 Lin. Date: 07/06/2010 Lin. No.: 00009
Solution File No.: 01480 Soln. Date: 08/06/2010 Soln. No.: 00128
Sequential File No.: 01480 File Date: 08/06/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0341
Control Solution %: 0.100% Expires: 09/18/2011
Solution Control Lot: 09IO69 Bottle No.: 0026

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:27D		
Control 1 EC	0.101%	10:27D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:28D		
Control 2 EC	0.100%	10:29D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	10:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:29D		
Control 3 EC	0.100%	10:30D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	10:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:31D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature: 

Badge No.: 127

Date: 08/06/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01460	Calib. Date: 07/06/2010
Certification File No.:	01461	Calib. No.: 00011
Linearity File No.:	01462	Cert. Date: 07/06/2010
Solution File No.:	01496	Cert. No.: 00009
Sequential File No.:	01496	Lin. Date: 07/06/2010
		Lin. No.: 00009
		Soln. Date: 08/20/2010
		Soln. No.: 00129
		File Date: 08/20/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0341
Solution Control Lot:	09I069	Expires: 09/18/2011
		Bottle No.: 0019

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:28D		
Control 1 EC	0.101%	11:29D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:30D		
Control 2 EC	0.100%	11:30D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	11:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:31D		
Control 3 EC	0.100%	11:31D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:32D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: .

First Name: CHRIS

MI: L

Signature: _____



Badge No.: 127

Date: 08/20/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01460	Calib. Date: 07/06/2010
Certification File No.:	01461	Calib. No.: 00011
Linearity File No.:	01462	Cert. Date: 07/06/2010
Solution File No.:	01514	Cert. No.: 00009
Sequential File No.:	01514	Lin. Date: 07/06/2010
		Lin. No.: 00009
		Soln. Date: 10/02/2010
		Soln. No.: 00130
		File Date: 10/02/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0341
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 0560

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:49D		
Control 1 EC	0.102%	15:50D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	15:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:50D		
Control 2 EC	0.101%	15:51D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	15:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:52D		
Control 3 EC	0.101%	15:52D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	15:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:53D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KILLION

First Name: MICHAEL

MI: P.

Signature: _____

Det. M. Killion #170
 Det. M. Killion #170

Badge No.: 170

Date: 10/02/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	01460	Calib. Date:	07/06/2010
Certification File No.:	01461	Cert. No.:	00011
Linearity File No.:	01462	Cert. Date:	07/06/2010
Solution File No.:	01521	Lin. Date:	07/06/2010
Sequential File No.:	01521	Lin. No.:	00009
		Soln. Date:	10/29/2010
		Soln. No.:	00131
		File Date:	10/29/2010
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0341
Solution Control Lot:	10C077	Expires:	03/10/2012
		Bottle No.:	0569

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:29D		
Control 1 EC	0.102%	17:30D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	17:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:31D		
Control 2 EC	0.101%	17:31D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	17:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:32D		
Control 3 EC	0.100%	17:32D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	17:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:33D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KERN

First Name: RAYMOND

MI: T

Signature: _____

For R Kern #181

Badge No.: 181

Date: 10/29/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01460	Calib. Date: 07/06/2010
Certification File No.:	01461	Calib. No.: 00011
Linearity File No.:	01462	Cert. Date: 07/06/2010
Solution File No.:	01536	Cert. No.: 00009
Sequential File No.:	01536	Lin. Date: 07/06/2010
		Lin. No.: 00009
		Soln. Date: 11/24/2010
		Soln. No.: 00132
		File Date: 11/24/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0341
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 0565

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:01S		
Control 1 EC	0.101%	11:02S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	11:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:03S		
Control 2 EC	0.100%	11:03S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	11:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:04S		
Control 3 EC	0.101%	11:05S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	11:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:06S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: *Gerald Henkel 149*

Badge No.: 149

Date: 11/24/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01460	Calib. Date: 07/06/2010
Certification File No.:	01461	Calib. No.: 00011
Linearity File No.:	01462	Cert. Date: 07/06/2010
Solution File No.:	01556	Cert. No.: 00009
Sequential File No.:	01556	Lin. Date: 07/06/2010
		Lin. No.: 00009
		Soln. Date: 12/18/2010
		Soln. No.: 00133
		File Date: 12/18/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0341
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 0564

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:36S		
Control 1 EC	0.104%	02:36S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	02:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:37S		
Control 2 EC	0.101%	02:38S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	02:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:39S		
Control 3 EC	0.101%	02:39S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	02:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:40S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____

PH M Henkel 149

Badge No.: 149

Date: 12/18/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	Calib. No.:	00012
Calibration File No.:	01557	Cert. Date:	12/22/2010
Certification File No.:	01558	Lin. Date:	12/22/2010
Linearity File No.:	01559	Soln. Date:	12/31/2010
Solution File No.:	01568	File Date:	12/31/2010
Sequential File No.:	01568		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0341
Solution Control Lot:	10C077	Expires:	03/10/2012
		Bottle No.:	0563

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:55S		
Control 1 EC	0.102%	11:55S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	11:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:56S		
Control 2 EC	0.100%	11:57S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	11:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:58S		
Control 3 EC	0.100%	11:58S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	11:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:59S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature: _____

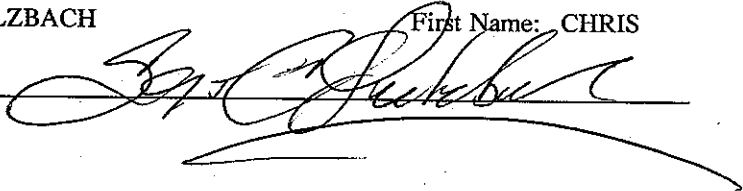

Badge No.: 127

Date: 12/31/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	01557	Calib. Date:	12/22/2010
Certification File No.:	01558	Cert. No.:	00012
Linearity File No.:	01559	Cert. Date:	12/22/2010
Solution File No.:	01584	Lin. Date:	12/22/2010
Sequential File No.:	01584	Soln. Date:	01/17/2011
		File Date:	01/17/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0341
Solution Control Lot:	10C077	Expires:	03/10/2012
		Bottle No.:	0554

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:15S		
Control 1 EC	0.101%	09:16S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	09:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:17S		
Control 2 EC	0.100%	09:17S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	09:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:18S		
Control 3 EC	0.100%	09:19S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:19S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:20S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature: _____

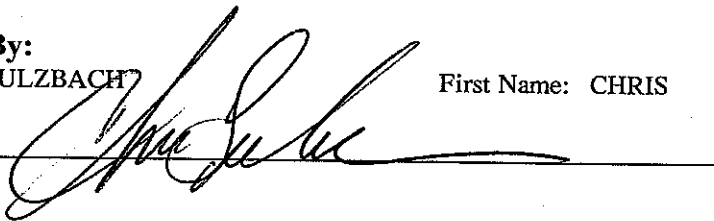

Badge No.: 127

Date: 01/17/2011

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01557	Calib. Date: 12/22/2010
Certification File No.:	01558	Calib. No.: 00012
Linearity File No.:	01559	Cert. Date: 12/22/2010
Solution File No.:	01593	Cert. No.: 00010
Sequential File No.:	01593	Lin. Date: 12/22/2010
		Lin. No.: 00010
		Soln. Date: 01/26/2011
		Soln. No.: 00138
		File Date: 01/26/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0341
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 0566

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:41S		
Control 1 EC	0.101%	10:42S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	10:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:43S		
Control 2 EC	0.100%	10:43S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	10:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:44S		
Control 3 EC	0.100%	10:45S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:45S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:46S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature: _____



Badge No.: 127

Date: 01/26/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01557	Calib. Date: 12/22/2010
Certification File No.:	01558	Calib. No.: 00012
Linearity File No.:	01559	Cert. Date: 12/22/2010
Solution File No.:	01605	Cert. No.: 00010
Sequential File No.:	01605	Lin. Date: 12/22/2010
		Lin. No.: 00010
		Soln. Date: 02/06/2011
		Soln. No.: 00139
		File Date: 02/06/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0341
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 0557

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:38S		
Control 1 EC	0.101%	09:38S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:39S		
Control 2 EC	0.100%	09:40S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	09:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:41S		
Control 3 EC	0.099%	09:41S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:42S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature: _____

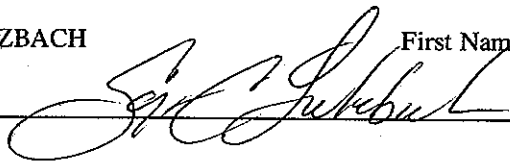

Badge No.: 127

Date: 02/06/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	01557	Calib. Date:	12/22/2010
Certification File No.:	01558	Cert. Date:	12/22/2010
Linearity File No.:	01559	Lin. Date:	12/22/2010
Solution File No.:	01614	Soln. Date:	02/16/2011
Sequential File No.:	01614	File Date:	02/16/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0341
Solution Control Lot:	10C077	Expires:	03/10/2012
		Bottle No.:	0562

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:05S		
Control 1 EC	0.101%	00:05S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	00:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:06S		
Control 2 EC	0.099%	00:07S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	00:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:08S		
Control 3 EC	0.099%	00:08S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	00:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:09S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KERN

First Name: RAYMOND

MI: T

Signature: _____

Ray Kern #181

Badge No.: 181

Date: 02/16/2011

Calibrating Unit New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C		Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.		
Calibration File No.: 01557	Calib. Date: 12/22/2010	Calib. No.: 00012
Certification File No.: 01558	Cert. Date: 12/22/2010	Cert. No.: 00010
Linearity File No.: 01559	Lin. Date: 12/22/2010	Lin. No.: 00010
Solution File No.: 01621	Soln. Date: 02/19/2011	Soln. No.: 00141
Sequential File No.: 01621	File Date: 02/19/2011	

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUN S3-0341
Control Solution %: 0.100%		Expires: 03/10/2012
Solution Control Lot: 10C077		Bottle No.: 0567

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	21:45S		
Control 1 EC	0.100%	21:45S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	21:45S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:46S		
Control 2 EC	0.099%	21:47S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	21:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:48S		
Control 3 EC	0.100%	21:48S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	21:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:49S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KERN

First Name: RAYMOND

MI: T

Signature: _____

Ray Kern #181

Badge No.: 181

Date: 02/19/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	01557	Calib. Date:	12/22/2010
Certification File No.:	01558	Cert. No.:	00012
Linearity File No.:	01559	Cert. Date:	12/22/2010
Solution File No.:	01633	Lin. No.:	00010
Sequential File No.:	01633	Lin. Date:	12/22/2010
		Soln. No.:	00142
		Soln. Date:	02/24/2011
		File Date:	02/24/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0341
Solution Control Lot:	10C077	Expires:	03/10/2012
		Bottle No.:	0551

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:34S		
Control 1 EC	0.100%	03:34S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	03:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:35S		
Control 2 EC	0.098%	03:36S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	03:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:37S		
Control 3 EC	0.097%	03:37S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	03:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:38S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MOLES

First Name: VITO

MI: M

Signature: _____

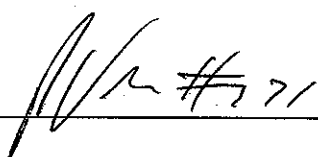

Badge No.: 171

Date: 02/24/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01557	Calib. Date: 12/22/2010
Certification File No.:	01558	Calib. No.: 00012
Linearity File No.:	01559	Cert. Date: 12/22/2010
Solution File No.:	01635	Cert. No.: 00010
Sequential File No.:	01635	Lin. Date: 12/22/2010
		Lin. No.: 00010
		Soln. Date: 02/25/2011
		Soln. No.: 00143
		File Date: 02/25/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0341
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 0571

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:48S		
Control 1 EC	0.100%	13:49S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:50S		
Control 2 EC	0.098%	13:50S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	13:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:51S		
Control 3 EC	0.099%	13:52S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:53S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature: _____

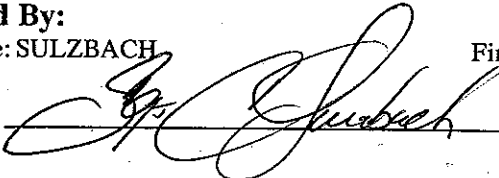

Badge No.: 127

Date: 02/25/2011