

# Alcotest 7110 Calibration Record

**Equipment**

Alcotest 7110 MKIII-C  
Location: PENNSAUKEN TWSP. P.D. Serial No.: ARUM-0066  
Calibration File No.: 02271 Calib. Date: 07/11/2017 Calib. No.: 00031  
Certification File No.: 02176 Cert. Date: 01/11/2017 Cert. No.: 00026  
Linearity File No.: 02177 Lin. Date: 01/11/2017 Lin. No.: 00026  
Solution File No.: 02265 Soln. Date: 07/02/2017 Soln. No.: 00234  
Sequential File No.: 02271 File Date: 07/11/2017


Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0340  
Control Solution %: 0.100% Expires: 10/10/2018  
Solution Control Lot: 16270 Bottle No.: 1306

**Coordinator**

Last Name: WATSON First Name: MATTHEW MI: R  
Signature: Tpr. # [Signature] #7078 Badge No.: 7078  
Date: 07/11/2017

\*Black Key Temperature Probe Serial.....# DDXKP2-390 (MRW)  
\*Digital NIST Temperature Measuring System Serial.....# 15AG71438 (MRW)

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

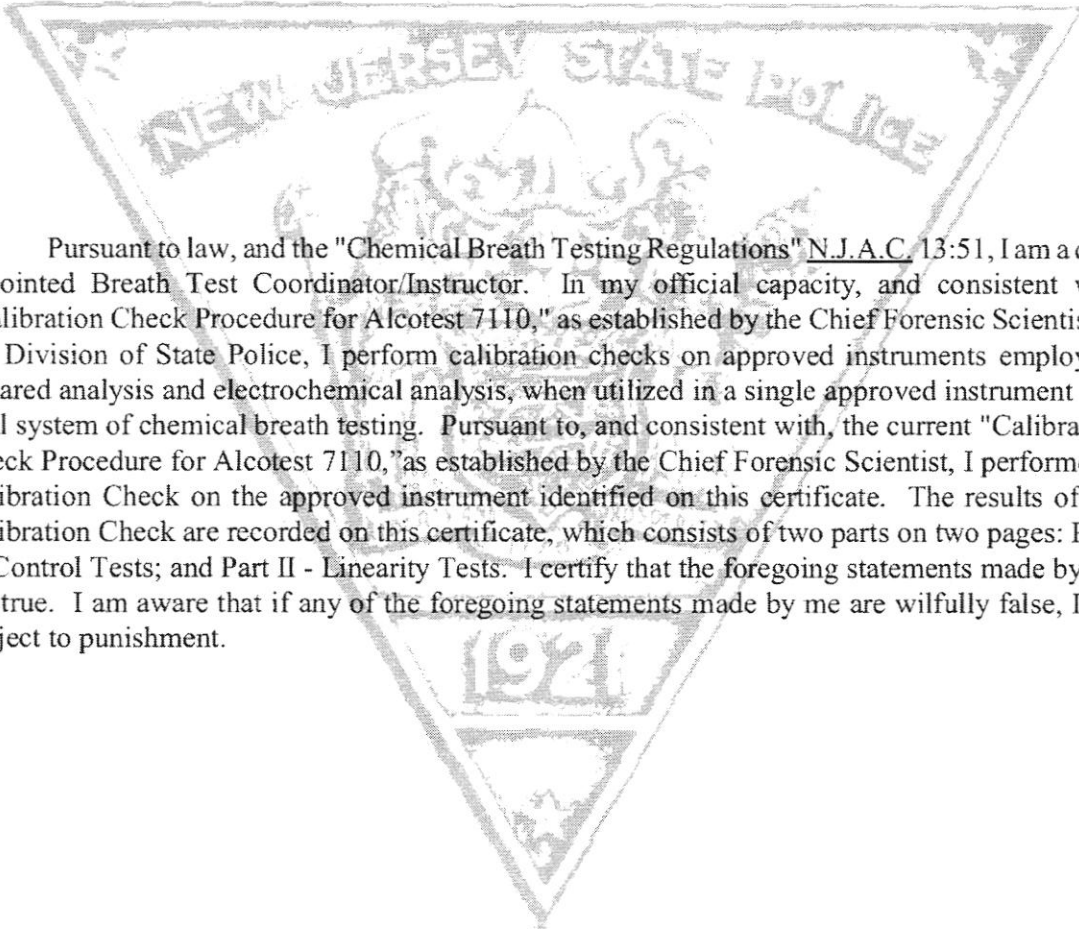

# Alcotest 7110 Calibration Certificate

## Part I - Control Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARUM-0066  
Location: PENNSAUKEN TWSP. P.D.  
Calibration File No.: 02271 Calib. Date: 07/11/2017 Calib. No.: 00031  
Certification File No.: 02272 Cert. Date: 07/11/2017 Cert. No.: 00027  
Linearity File No.: 02177 Lin. Date: 01/11/2017 Lin. No.: 00026  
Solution File No.: 02265 Soln. Date: 07/02/2017 Soln. No.: 00234  
Sequential File No.: 02272 File Date: 07/11/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0340  
Control Solution %: 0.100% Expires: 10/10/2018  
Solution Control Lot: 16270 Bottle No.: 1306

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:18D		
Control 1 EC	0.099%	09:19D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:19D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:20D		
Control 2 EC	0.099%	09:20D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:21D		
Control 3 EC	0.099%	09:22D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:22D		


All tests within acceptable tolerance.

### Coordinator

Last Name: WATSON

First Name: MATTHEW

MI: R

Signature:  #7078

Badge No.: 7078

Date: 07/11/2017

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.