

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01119	Calib. Date: 07/28/2011
Certification File No.:	01120	Calib. No.: 00017
Linearity File No.:	01121	Cert. Date: 07/28/2011
Solution File No.:	01219	Lin. No.: 00014
Sequential File No.:	01219	Lin. Date: 07/28/2011
		Soln. No.: 00119
		Soln. Date: 12/14/2011
		File Date: 12/14/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0339
Solution Control Lot:	11C088	Expires: 03/31/2013
		Bottle No.: 0188

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:00S		
Control 1 EC	0.101%	00:00S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	00:00S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:01S		
Control 2 EC	0.102%	00:02S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	00:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:02S		
Control 3 EC	0.101%	00:03S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.103%	00:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:04S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____

PK M Henkel 149

Badge No.: 149

Date: 12/14/2011

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C		Serial No.: ARUM-0066
Location: PENNSAUKEN TWSP. P.D.		
Calibration File No.: 01119	Calib. Date: 07/28/2011	Calib. No.: 00017
Certification File No.: 01120	Cert. Date: 07/28/2011	Cert. No.: 00014
Linearity File No.: 01121	Lin. Date: 07/28/2011	Lin. No.: 00014
Solution File No.: 01218	Soln. Date: 12/13/2011	Soln. No.: 00118
Sequential File No.: 01218	File Date: 12/13/2011	
Calibrating Unit: WET	Model No.: CU-34	Serial No.:]
Control Solution %: 0.100%		Expires: 03/31/2013
Solution Control Lot: 11C088		Bottle No.: 0183

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:59S		
Control 1 EC	0.102%	21:00S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	21:00S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:01S		
Control 2 EC	0.101%	21:01S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	21:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:02S		
Control 3 EC	0.101%	21:03S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	21:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:03S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____

PK M Henkel 149

Badge No.: 149

Date: 12/13/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0066
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01119 Calib. Date: 07/28/2011 Calib. No.: 00017
Certification File No.: 01120 Cert. Date: 07/28/2011 Cert. No.: 00014
Linearity File No.: 01121 Lin. Date: 07/28/2011 Lin. No.: 00014
Solution File No.: 01200 Soln. Date: 11/23/2011 Soln. No.: 00117
Sequential File No.: 01200 File Date: 11/23/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0339
Control Solution %: 0.100% Expires: 03/31/2013
Solution Control Lot: 11C088 Bottle No.: 0190

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:11S		
Control 1 EC	0.101%	09:12S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:13S		
Control 2 EC	0.101%	09:13S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	09:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:14S		
Control 3 EC	0.101%	09:15S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	09:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:15S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature: _____



Badge No.: 127

Date: 11/23/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0066
Location: PENNSAUKEN TWSP, P.D.
Calibration File No.: 01119 Calib. Date: 07/28/2011 Calib. No.: 00017
Certification File No.: 01120 Cert. Date: 07/28/2011 Cert. No.: 00014
Linearity File No.: 01121 Lin. Date: 07/28/2011 Lin. No.: 00014
Solution File No.: 01187 Soln. Date: 11/06/2011 Soln. No.: 00116
Sequential File No.: 01187 File Date: 11/06/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0339
Control Solution %: 0.100% Expires: 03/31/2013
Solution Control Lot: 11C088 Bottle No.: 0184

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:09S		
Control 1 EC	0.102%	18:10S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	18:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:10S		
Control 2 EC	0.101%	18:11S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	18:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:12S		
Control 3 EC	0.101%	18:12S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	18:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:13S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: 

149

Badge No.: 149

Date: 11/06/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0066
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01119 Calib. Date: 07/28/2011 Calib. No.: 00017
Certification File No.: 01120 Cert. Date: 07/28/2011 Cert. No.: 00014
Linearity File No.: 01121 Lin. Date: 07/28/2011 Lin. No.: 00014
Solution File No.: 01186 Soln. Date: 11/06/2011 Soln. No.: 00115
Sequential File No.: 01186 File Date: 11/06/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0339
Control Solution %: 0.100% Expires: 03/31/2013
Solution Control Lot: 11C088 Bottle No.: 0189

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:40S		
Control 1 EC	-.---%	03:41S	22.0°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	03:41S	22.0°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: 

149

Badge No.: 149

Date: 11/06/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0066
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01119 Calib. Date: 07/28/2011 Calib. No.: 00017
Certification File No.: 01120 Cert. Date: 07/28/2011 Cert. No.: 00014
Linearity File No.: 01121 Lin. Date: 07/28/2011 Lin. No.: 00014
Solution File No.: 01171 Soln. Date: 10/10/2011 Soln. No.: 00114
Sequential File No.: 01171 File Date: 10/10/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0339
Control Solution %: 0.100% Expires: 10/04/2012
Solution Control Lot: 10J083 Bottle No.: 1180

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:27D		
Control 1 EC	0.101%	00:28D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	00:28D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:29D		
Control 2 EC	0.100%	00:29D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	00:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:30D		
Control 3 EC	0.100%	00:30D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	00:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:31D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____



Badge No.: 149

Date: 10/10/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01119	Calib. Date: 07/28/2011
Certification File No.:	01120	Calib. No.: 00017
Linearity File No.:	01121	Cert. Date: 07/28/2011
Solution File No.:	01155	Lin. No.: 00014
Sequential File No.:	01155	Soln. Date: 09/17/2011
		Soln. No.: 00113
		File Date: 09/17/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0339
Solution Control Lot:	10J083	Expires: 10/04/2012
		Bottle No.: 1185

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:43D		
Control 1 EC	0.100%	04:44D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	04:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:44D		
Control 2 EC	0.100%	04:45D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	04:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:46D		
Control 3 EC	0.100%	04:46D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	04:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:47D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CIACCIA

First Name: MICHAEL

MI: -

Signature: _____



Badge No.: 172

Date: 09/17/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01119	Calib. Date: 07/28/2011
Certification File No.:	01120	Calib. No.: 00017
Linearity File No.:	01121	Cert. Date: 07/28/2011
Solution File No.:	01136	Cert. No.: 00014
Sequential File No.:	01136	Lin. Date: 07/28/2011
		Lin. No.: 00014
		Soln. Date: 08/25/2011
		Soln. No.: 00112
		File Date: 08/25/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0339
Solution Control Lot:	10J083	Expires: 10/04/2012
		Bottle No.: 1176

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	04:00D		
Control 1 EC	0.100%	04:01D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	04:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:01D		
Control 2 EC	0.100%	04:02D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	04:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:03D		
Control 3 EC	0.100%	04:03D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	04:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:04D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HARTNETT

First Name: JAMES

MI: /

Signature: _____

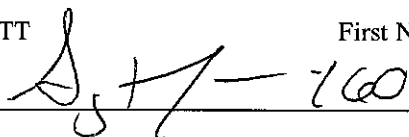

Badge No.: 160

Date: 08/25/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01083	Calib. Date: 06/16/2011
Certification File No.:	01084	Calib. No.: 00016
Linearity File No.:	01085	Cert. Date: 06/16/2011
Solution File No.:	01117	Cert. No.: 00013
Sequential File No.:	01117	Lin. Date: 06/16/2011
		Lin. No.: 00013
		Soln. Date: 07/22/2011
		Soln. No.: 00110
		File Date: 07/22/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0339
Solution Control Lot:	10J083	Expires: 10/04/2012
		Bottle No.: 1182

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:44D		
Control 1 EC	0.097%	00:45D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	00:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:46D		
Control 2 EC	0.096%	00:46D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	00:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:47D		
Control 3 EC	0.097%	00:48D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	00:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:48D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____

G. Henkel 149

Badge No.: 149

Date: 07/22/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0066
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01083 Calib. Date: 06/16/2011 Calib. No.: 00016
Certification File No.: 01084 Cert. Date: 06/16/2011 Cert. No.: 00013
Linearity File No.: 01085 Lin. Date: 06/16/2011 Lin. No.: 00013
Solution File No.: 01110 Soln. Date: 07/12/2011 Soln. No.: 00109
Sequential File No.: 01110 File Date: 07/12/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0339
Control Solution %: 0.100% Expires: 10/04/2012
Solution Control Lot: 10J083 Bottle No.: 1186

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:45D		
Control 1 EC	0.098%	00:46D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	00:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:46D		
Control 2 EC	0.097%	00:47D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	00:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:48D		
Control 3 EC	0.097%	00:48D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	00:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:49D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: *He M Henkel 149*

Badge No.: 149

Date: 07/12/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0066
Location: PENNSAUKEN TWSP, P.D.
Calibration File No.: 01083 Calib. Date: 06/16/2011 Calib. No.: 00016
Certification File No.: 01084 Cert. Date: 06/16/2011 Cert. No.: 00013
Linearity File No.: 01085 Lin. Date: 06/16/2011 Lin. No.: 00013
Solution File No.: 01105 Soln. Date: 07/02/2011 Soln. No.: 00108
Sequential File No.: 01105 File Date: 07/02/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0339
Control Solution %: 0.100% Expires: 10/04/2012
Solution Control Lot: 10J083 Bottle No.: 1181

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:36D		
Control 1 EC	0.098%	16:37D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	16:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:37D		
Control 2 EC	0.097%	16:38D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	16:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:38D		
Control 3 EC	0.098%	16:39D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	16:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:40D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SANDERS

First Name: JAMES

MI: R

Signature: 

Badge No.: 126

Date: 07/02/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	01083	Calib. Date:	06/16/2011
Certification File No.:	01084	Cert. Date:	06/16/2011
Linearity File No.:	01085	Lin. Date:	06/16/2011
Solution File No.:	01097	Soln. Date:	06/25/2011
Sequential File No.:	01097	File Date:	06/25/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0339
Solution Control Lot:	10J083	Expires:	10/04/2012
		Bottle No.:	1191

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:36D		
Control 1 EC	0.097%	00:37D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.096%	00:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:37D		
Control 2 EC	0.096%	00:38D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.096%	00:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:38D		
Control 3 EC	0.097%	00:39D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.096%	00:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:40D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KERN

First Name: RAYMOND

MI: T

Signature: _____

Ray Kern #181

Badge No.: 181

Date: 06/25/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	00972	Calib. Date: 03/01/2011
Certification File No.:	00973	Calib. No.: 00015
Linearity File No.:	00974	Cert. Date: 03/01/2011
Solution File No.:	01069	Cert. No.: 00012
Sequential File No.:	01069	Lin. Date: 03/01/2011
		Lin. No.: 00012
		Soln. Date: 05/27/2011
		Soln. No.: 00105
		File Date: 05/27/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	10J083	Expires: 10/04/2012
		Bottle No.: 1188

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:57D		
Control 1 EC	0.099%	09:58D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:58D		
Control 2 EC	0.099%	09:59D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:00D		
Control 3 EC	0.099%	10:00D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	10:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:01D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature: _____



Badge No.: 127

Date: 05/27/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	00972	Calib. Date:	03/01/2011
Certification File No.:	00973	Cert. No.:	00015
Linearity File No.:	00974	Cert. Date:	03/01/2011
Solution File No.:	01049	Lin. No.:	00012
Sequential File No.:	01049	Lin. Date:	03/01/2011
		Soln. No.:	00104
		Soln. Date:	05/07/2011
		File Date:	05/07/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0338
Solution Control Lot:	10J083	Expires:	10/04/2012
		Bottle No.:	1192

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	00:56D		
Control 1 EC	0.101%	00:56D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	00:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:57D		
Control 2 EC	0.100%	00:57D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	00:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:58D		
Control 3 EC	0.100%	00:59D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	00:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:59D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: *De M Henkel 149*

Badge No.: 149

Date: 05/07/2011

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
PENNSAUKEN TWSP. P.D. Serial No.: ARUM-0066

Location: Calib. Date: 03/01/2011 Calib. No.: 00015
Calibration File No.: 00972 Cert. Date: 03/01/2011 Cert. No.: 00012
Certification File No.: 00973 Lin. Date: 03/01/2011 Lin. No.: 00012
Linearity File No.: 00974 Soln. Date: 04/16/2011 Soln. No.: 00103
Solution File No.: 01034 File Date: 04/16/2011

Sequential File No.: 01034

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0338
Control Solution %: 0.100% Expires: 10/04/2012
Solution Control Lot: 10J083 Bottle No.: 1200

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:44D		
Control 1 EC	0.101%	16:45D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	16:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:46D		
Control 2 EC	0.101%	16:46D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	16:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:47D		
Control 3 EC	0.101%	16:48D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	16:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:48D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: KERN

First Name: RAYMOND

MI: T

Signature: _____



Badge No.: 181

Date: 04/16/2011

Calibrating Unit New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location: PENNSAUKEN TWSP. P.D.	
Calibration File No.: 00972	Calib. Date: 03/01/2011
Certification File No.: 00973	Cert. No.: 00015
Linearity File No.: 00974	Cert. Date: 03/01/2011
Solution File No.: 01014	Lin. No.: 00012
Sequential File No.: 01014	Lin. Date: 03/01/2011
	Soln. Date: 04/05/2011
	Soln. No.: 00102
	File Date: 04/05/2011

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUN S3-0338
Control Solution %: 0.100%		Expires: 10/04/2012
Solution Control Lot: 10J083		Bottle No.: 1199

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	22:31D		
Control 1 EC	0.101%	22:32D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	22:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:32D		
Control 2 EC	0.101%	22:33D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	22:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:34D		
Control 3 EC	0.102%	22:34D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	22:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:35D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____

[Handwritten Signature: G. M. Henkel] *[Handwritten Initials: H19]*

Badge No.: 149

Date: 04/05/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	00942	Calib. Date: 12/22/2010
Certification File No.:	00943	Calib. No.: 00012
Linearity File No.:	00944	Cert. Date: 12/22/2010
Solution File No.:	00965	Cert. No.: 00011
Sequential File No.:	00965	Lin. Date: 12/22/2010
		Lin. No.: 00011
		Soln. Date: 02/06/2011
		Soln. No.: 00097
		File Date: 02/06/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 0573

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:39S		
Control 1 EC	0.102%	09:39S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:40S		
Control 2 EC	0.097%	09:41S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	09:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:42S		
Control 3 EC	0.098%	09:42S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:43S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature: _____

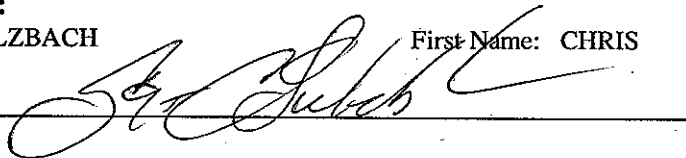

Badge No.: 127

Date: 02/06/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	00942	Calib. Date:	12/22/2010
Certification File No.:	00943	Cert. Date:	12/22/2010
Linearity File No.:	00944	Lin. Date:	12/22/2010
Solution File No.:	00957	Soln. Date:	01/24/2011
Sequential File No.:	00957	File Date:	01/24/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0338
Solution Control Lot:	10C077	Expires:	03/10/2012
		Bottle No.:	0561

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:16S		
Control 1 EC	0.101%	08:17S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:18S		
Control 2 EC	0.096%	08:18S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:19S		
Control 3 EC	0.098%	08:20S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:20S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:21S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KUCHMEK

First Name: JOSEPH

MI: -

Signature: _____

PJ

#190

Badge No.: 190

Date: 01/24/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	00942	Calib. Date: 12/22/2010
Certification File No.:	00943	Calib. No.: 00012
Linearity File No.:	00944	Cert. Date: 12/22/2010
Solution File No.:	00954	Cert. No.: 00011
Sequential File No.:	00954	Lin. Date: 12/22/2010
		Lin. No.: 00011
		Soln. Date: 01/17/2011
		Soln. No.: 00095
		File Date: 01/17/2011

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUN S3-0338
Control Solution %: 0.100%		Expires: 03/10/2012
Solution Control Lot: 10C077		Bottle No.: 0556

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:04S		
Control 1 EC	0.101%	08:05S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:06S		
Control 2 EC	0.097%	08:06S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:07S		
Control 3 EC	0.098%	08:08S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:09S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____

[Handwritten Signature] 149

Badge No.: 149

Date: 01/17/2011