

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02003	Calib. Date: 09/09/2015
Certification File No.:	02004	Calib. No.: 00026
Linearity File No.:	02005	Cert. Date: 09/09/2015
Solution File No.:	02038	Cert. No.: 00023
Sequential File No.:	02038	Lin. Date: 09/09/2015
		Lin. No.: 00023
		Soln. Date: 01/17/2016
		Soln. No.: 00197
		File Date: 01/17/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0341
Solution Control Lot:	14L135	Expires: 12/31/2016
		Bottle No.: 0064

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:45S		
Control 1 EC	0.102%	09:46S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:46S		
Control 2 EC	0.100%	09:47S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	09:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:48S		
Control 3 EC	0.100%	09:49S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:50S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KERN

First Name: RAYMOND

MI: T

Signature: _____

R Kern #181

Badge No.: 181

Date: 01/17/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02003	Calib. Date:	09/09/2015
Certification File No.:	02004	Cert. Date:	09/09/2015
Linearity File No.:	02005	Lin. Date:	09/09/2015
Solution File No.:	02040	Soln. Date:	01/29/2016
Sequential File No.:	02040	File Date:	01/29/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0341
Solution Control Lot:	14L135	Expires:	12/31/2016
		Bottle No.:	0067

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:38S		
Control 1 EC	0.102%	10:39S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:40S		
Control 2 EC	0.098%	10:40S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:41S		
Control 3 EC	0.097%	10:42S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	10:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:43S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____

[Handwritten Signature] 1/29/16

Badge No.: 187

Date: 01/29/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02003	Calib. Date: 09/09/2015
Certification File No.:	02004	Calib. No.: 00026
Linearity File No.:	02005	Cert. Date: 09/09/2015
Solution File No.:	02051	Cert. No.: 00023
Sequential File No.:	02051	Lin. Date: 09/09/2015
		Lin. No.: 00023
		Soln. Date: 02/11/2016
		Soln. No.: 00199
		File Date: 02/11/2016

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUN S3-0341
Control Solution %: 0.100%		Expires: 12/31/2016
Solution Control Lot: 14L135		Bottle No.: 0069

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:51S		
Control 1 EC	0.101%	03:52S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	03:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:53S		
Control 2 EC	0.100%	03:54S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	03:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:54S		
Control 3 EC	0.100%	03:55S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	03:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:56S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HARTNETT

First Name: JAMES

MI: J

Signature: _____

LHJ - 160

Badge No.: 160

Date: 02/11/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02003	Calib. Date: 09/09/2015
Certification File No.:	02004	Calib. No.: 00026
Linearity File No.:	02005	Cert. Date: 09/09/2015
Solution File No.:	02056	Cert. No.: 00023
Sequential File No.:	02056	Lin. Date: 09/09/2015
		Lin. No.: 00023
		Soln. Date: 02/15/2016
		Soln. No.: 00200
		File Date: 02/15/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0341
Solution Control Lot:	14L135	Expires: 12/31/2016
		Bottle No.: 0071

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	00:12S		
Control 1 EC	0.101%	00:13S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	00:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:14S		
Control 2 EC	0.099%	00:15S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	00:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:16S		
Control 3 EC	0.098%	00:16S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	00:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:17S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____

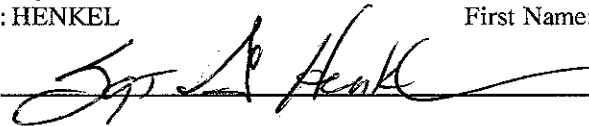

Badge No.: 149

Date: 02/15/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02003	Calib. Date: 09/09/2015
Certification File No.:	02004	Calib. No.: 00026
Linearity File No.:	02005	Cert. Date: 09/09/2015
Solution File No.:	02059	Cert. No.: 00023
Sequential File No.:	02059	Lin. Date: 09/09/2015
		Lin. No.: 00023
		Soln. Date: 02/20/2016
		Soln. No.: 00201
		File Date: 02/20/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0341
Solution Control Lot:	14L135	Expires: 12/31/2016
		Bottle No.: 0073

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:07S		
Control 1 EC	0.101%	08:07S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	08:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:08S		
Control 2 EC	0.100%	08:09S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:10S		
Control 3 EC	0.098%	08:11S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:12S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____

Badge No.: 187

Date: 02/20/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02003	Calib. Date:	09/09/2015
Certification File No.:	02004	Cert. No.:	00026
Linearity File No.:	02005	Cert. Date:	09/09/2015
Solution File No.:	02064	Lin. Date:	09/09/2015
Sequential File No.:	02064	Lin. No.:	00023
		Soln. Date:	02/24/2016
		Soln. No.:	00202
		File Date:	02/24/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0341
Solution Control Lot:	16A150	Expires:	01/05/2017
		Bottle No.:	1086

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:33S		
Control 1 EC	0.101%	10:34S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	10:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:35S		
Control 2 EC	0.101%	10:35S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	10:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:36S		
Control 3 EC	0.099%	10:37S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	10:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:38S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature:  #157

Badge No.: 187

Date: 02/24/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02068	Calib. Date: 03/01/2016
Certification File No.:	02069	Calib. No.: 00027
Linearity File No.:	02070	Cert. Date: 03/01/2016
Solution File No.:	02074	Cert. No.: 00024
Sequential File No.:	02074	Lin. Date: 03/01/2016
		Lin. No.: 00024
		Soln. Date: 03/10/2016
		Soln. No.: 00204
		File Date: 03/10/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0341
Solution Control Lot:	16A150	Expires: 01/05/2017
		Bottle No.: 1048

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:57S		
Control 1 EC	0.099%	15:58S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	15:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:59S		
Control 2 EC	0.097%	15:59S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	15:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:00S		
Control 3 EC	0.097%	16:01S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	16:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:02S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____



Badge No.: 187

Date: 03/10/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02068	Calib. Date:	03/01/2016
Certification File No.:	02069	Cert. No.:	00027
Linearity File No.:	02070	Cert. Date:	03/01/2016
Solution File No.:	02076	Lin. Date:	03/01/2016
Sequential File No.:	02076	Lin. No.:	00024
		Soln. Date:	03/17/2016
		Soln. No.:	00205
		File Date:	03/17/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0341
Solution Control Lot:	16A150	Expires:	01/05/2017
		Bottle No.:	1136

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:59S		
Control 1 EC	0.094%	20:59S	34.0°C	CONTROL TEST FAILED
Control 1 IR	0.095%	20:59S	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	21:00S		
Control 2 EC	0.092%	21:01S	34.0°C	CONTROL TEST FAILED
Control 2 IR	0.095%	21:01S	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	21:02S		
Control 3 EC	0.092%	21:03S	34.0°C	CONTROL TEST FAILED
Control 3 IR	0.096%	21:03S	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	21:04S		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____

Sgt M Henkel 179

Badge No.: 149

Date: 03/17/2016

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0066
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 02068 Calib. Date: 03/01/2016 Calib. No.: 00027
Certification File No.: 02069 Cert. Date: 03/01/2016 Cert. No.: 00024
Linearity File No.: 02070 Lin. Date: 03/01/2016 Lin. No.: 00024
Solution File No.: 02077 Soln. Date: 03/17/2016 Soln. No.: 00206
Sequential File No.: 02077 File Date: 03/17/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0341
Control Solution %: 0.100% Expires: 01/05/2017
Solution Control Lot: 16A150 Bottle No.: 1081

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:31S		
Control 1 EC	0.097%	23:32S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	23:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:33S		
Control 2 EC	0.093%	23:34S	34.0°C	CONTROL TEST FAILED
Control 2 IR	0.097%	23:34S	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	23:35S		
Control 3 EC	0.093%	23:35S	34.0°C	CONTROL TEST FAILED
Control 3 IR	0.096%	23:35S	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	23:36S		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____



Badge No.: 149

Date: 03/17/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02068	Calib. Date:	03/01/2016
Certification File No.:	02069	Cert. Date:	03/01/2016
Linearity File No.:	02070	Lin. Date:	03/01/2016
Solution File No.:	02078	Soln. Date:	03/18/2016
Sequential File No.:	02078	File Date:	03/18/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0341
Solution Control Lot:	16A150	Expires:	01/05/2017
		Bottle No.:	1043

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:53S		
Control 1 EC	0.098%	09:54S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:55S		
Control 2 EC	0.096%	09:56S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:56S		
Control 3 EC	0.097%	09:57S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:58S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature: _____

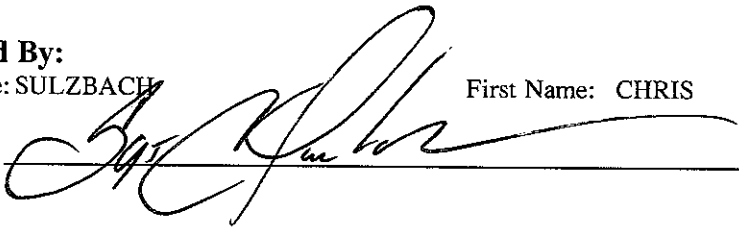

Badge No.: 127

Date: 03/18/2016

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0066
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 02068 Calib. Date: 03/01/2016 Calib. No.: 00027
Certification File No.: 02069 Cert. Date: 03/01/2016 Cert. No.: 00024
Linearity File No.: 02070 Lin. Date: 03/01/2016 Lin. No.: 00024
Solution File No.: 02080 Soln. Date: 03/23/2016 Soln. No.: 00208
Sequential File No.: 02080 File Date: 03/23/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0341
Control Solution %: 0.100% Expires: 01/05/2017
Solution Control Lot: 16A150 Bottle No.: 1272

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:22S		
Control 1 EC	0.101%	23:23S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	23:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:24S		
Control 2 EC	0.099%	23:25S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	23:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:25S		
Control 3 EC	0.099%	23:26S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	23:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:27S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____



Badge No.: 149

Date: 03/23/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02068	Calib. Date:	03/01/2016
Certification File No.:	02069	Cert. No.:	00027
Linearity File No.:	02070	Cert. Date:	03/01/2016
Solution File No.:	02082	Lin. Date:	03/01/2016
Sequential File No.:	02082	Lin. No.:	00024
		Soln. Date:	03/26/2016
		Soln. No.:	00209
		File Date:	03/26/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0341
Solution Control Lot:	14F130	Expires:	06/20/2016
		Bottle No.:	0739

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:30S		
Control 1 EC	0.100%	03:31S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	03:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:32S		
Control 2 EC	0.099%	03:32S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	03:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:33S		
Control 3 EC	0.098%	03:34S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	03:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:35S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HARTNETT

First Name: JAMES

MI: J

Signature: _____

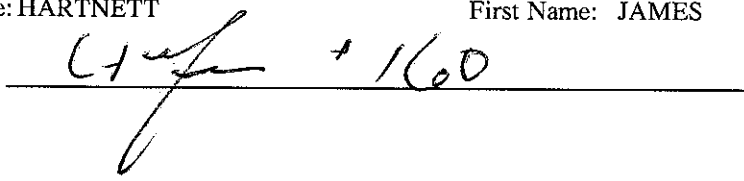

Badge No.: 160

Date: 03/26/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02068	Calib. Date: 03/01/2016
Certification File No.:	02069	Calib. No.: 00027
Linearity File No.:	02070	Cert. Date: 03/01/2016
Solution File No.:	02085	Cert. No.: 00024
Sequential File No.:	02085	Lin. Date: 03/01/2016
		Lin. No.: 00024
		Soln. Date: 03/29/2016
		Soln. No.: 00210
		File Date: 03/29/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0341
Solution Control Lot:	14F130	Expires: 06/20/2016
		Bottle No.: 0726

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:11S		
Control 1 EC	0.100%	02:12S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	02:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:13S		
Control 2 EC	0.099%	02:13S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	02:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:14S		
Control 3 EC	0.099%	02:15S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	02:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:16S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____

[Handwritten Signature] 187

Badge No.: 187

Date: 03/29/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02068	Calib. Date:	03/01/2016
Certification File No.:	02069	Cert. No.:	00027
Linearity File No.:	02070	Cert. Date:	03/01/2016
Solution File No.:	02087	Lin. No.:	00024
Sequential File No.:	02087	Lin. Date:	03/01/2016
		Soln. Date:	04/01/2016
		Soln. No.:	00211
		File Date:	04/01/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0341
Solution Control Lot:	14F130	Expires:	06/20/2016
		Bottle No.:	0744

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:41S		
Control 1 EC	0.098%	20:42S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:43S		
Control 2 EC	0.097%	20:43S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	20:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:44S		
Control 3 EC	0.097%	20:45S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	20:45S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:46S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BRISTOW

First Name: MAR

MI: V

Signature: PTL. Bristow #195

Badge No.: 0195

Date: 04/01/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02068	Calib. Date: 03/01/2016
Certification File No.:	02069	Calib. No.: 00027
Linearity File No.:	02070	Cert. Date: 03/01/2016
Solution File No.:	02089	Cert. No.: 00024
Sequential File No.:	02089	Lin. Date: 03/01/2016
		Lin. No.: 00024
		Soln. Date: 04/02/2016
		Soln. No.: 00212
		File Date: 04/02/2016

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0341
Solution Control Lot:	14F130	Expires: 06/20/2016
		Bottle No.: 0748

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:09S		
Control 1 EC	0.096%	06:09S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	06:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:10S		
Control 2 EC	0.095%	06:11S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	06:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:12S		
Control 3 EC	0.097%	06:12S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	06:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:13S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PASQUALE

First Name: J

MI:

Signature: 

Badge No.: 199

Date: 04/02/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0066
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 02068 Calib. Date: 03/01/2016 Calib. No.: 00027
Certification File No.: 02069 Cert. Date: 03/01/2016 Cert. No.: 00024
Linearity File No.: 02070 Lin. Date: 03/01/2016 Lin. No.: 00024
Solution File No.: 02085 Soln. Date: 03/29/2016 Soln. No.: 00210
Sequential File No.: 02085 File Date: 03/29/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0341
Control Solution %: 0.100% Expires: 06/20/2016
Solution Control Lot: 14F130 Bottle No.: 0726

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	02:11S		
Control 1 EC	0.100%	02:12S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	02:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:13S		
Control 2 EC	0.099%	02:13S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	02:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:14S		
Control 3 EC	0.099%	02:15S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	02:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:16S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____



Badge No.: 187

Date: 03/29/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02068	Calib. Date:	03/01/2016
Certification File No.:	02069	Cert. No.:	00027
Linearity File No.:	02070	Cert. Date:	03/01/2016
Solution File No.:	02102	Lin. No.:	00024
Sequential File No.:	02102	Lin. Date:	03/01/2016
		Soln. Date:	04/20/2016
		Soln. No.:	00213
		File Date:	04/20/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0341
Solution Control Lot:	16A150	Expires:	01/05/2017
		Bottle No.:	1287

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:23D		
Control 1 EC	0.100%	01:23D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	01:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:24D		
Control 2 EC	0.099%	01:25D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	01:25D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:26D		
Control 3 EC	0.097%	01:26D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	01:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:27D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SEXTON

First Name: RYAN

MI: G

Signature: *PM [Signature]* #206

Badge No.: 206

Date: 04/20/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02068	Calib. Date: 03/01/2016
Certification File No.:	02069	Calib. No.: 00027
Linearity File No.:	02070	Cert. Date: 03/01/2016
Solution File No.:	02105	Cert. No.: 00024
Sequential File No.:	02105	Lin. Date: 03/01/2016
		Lin. No.: 00024
		Soln. Date: 04/25/2016
		Soln. No.: 00214
		File Date: 04/25/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0341
Solution Control Lot:	16A150	Expires: 01/05/2017
		Bottle No.: 1288

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:18D		
Control 1 EC	0.097%	16:18D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	16:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:19D		
Control 2 EC	0.097%	16:20D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	16:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:21D		
Control 3 EC	0.096%	16:22D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	16:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:22D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____



Badge No.: 187

Date: 04/25/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02068	Calib. Date: 03/01/2016
Certification File No.:	02069	Calib. No.: 00027
Linearity File No.:	02070	Cert. Date: 03/01/2016
Solution File No.:	02108	Cert. No.: 00024
Sequential File No.:	02108	Lin. Date: 03/01/2016
		Lin. No.: 00024
		Soln. Date: 04/30/2016
		Soln. No.: 00215
		File Date: 04/30/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0341
Solution Control Lot:	201603L	Expires: 03/22/2018
		Bottle No.: 0179

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:52D		
Control 1 EC	0.100%	11:52D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	11:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:53D		
Control 2 EC	0.099%	11:54D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:55D		
Control 3 EC	0.100%	11:55D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:56D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____



Badge No.: 187

Date: 04/30/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02068	Calib. Date:	03/01/2016
Certification File No.:	02069	Cert. No.:	00027
Linearity File No.:	02070	Lin. Date:	03/01/2016
Solution File No.:	02110	Cert. No.:	00024
Sequential File No.:	02110	Lin. No.:	00024
		Soln. Date:	05/09/2016
		Soln. No.:	00216
		File Date:	05/09/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0341
Solution Control Lot:	201603L	Expires:	03/22/2018
		Bottle No.:	0181

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:13D		
Control 1 EC	0.101%	13:13D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:14D		
Control 2 EC	0.100%	13:15D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:16D		
Control 3 EC	0.099%	13:16D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:17D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____

[Handwritten Signature] *187

Badge No.: 187

Date: 05/09/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02068	Calib. Date:	03/01/2016
Certification File No.:	02069	Cert. Date:	03/01/2016
Linearity File No.:	02070	Lin. Date:	03/01/2016
Solution File No.:	02112	Soln. Date:	05/14/2016
Sequential File No.:	02112	File Date:	05/14/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0341
Solution Control Lot:	201603L	Expires:	03/22/2018
		Bottle No.:	0182

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:02D		
Control 1 EC	0.000%	07:03D	34.0°C	CONTROL TEST FAILED
Control 1 IR	0.100%	07:03D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	07:03D		
Control 2 EC	0.000%	07:04D	34.0°C	CONTROL TEST FAILED
Control 2 IR	0.101%	07:04D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	07:04D		
Control 3 EC	0.000%	07:05D	34.0°C	CONTROL TEST FAILED
Control 3 IR	0.101%	07:05D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	07:06D		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BRISTOW

First Name: MARK

MI: V

Signature: PTL. BmB #195

Badge No.: 0195

Date: 05/14/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02068	Calib. Date:	03/01/2016
Certification File No.:	02069	Cert. No.:	00027
Linearity File No.:	02070	Cert. Date:	03/01/2016
Solution File No.:	02113	Lin. No.:	00024
Sequential File No.:	02113	Lin. Date:	03/01/2016
		Soln. No.:	00218
		Soln. Date:	05/14/2016
		File Date:	05/14/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0341
Solution Control Lot:	201603L	Expires:	03/22/2018
		Bottle No.:	0183

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:52D		
Control 1 EC	0.000%	08:53D	34.0°C	CONTROL TEST FAILED
Control 1 IR	0.100%	08:53D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	08:53D		
Control 2 EC	0.000%	08:54D	34.0°C	CONTROL TEST FAILED
Control 2 IR	0.100%	08:54D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	08:54D		
Control 3 EC	0.000%	08:55D	34.0°C	CONTROL TEST FAILED
Control 3 IR	0.099%	08:55D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	08:56D		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____

[Handwritten Signature] #187

Badge No.: 187

Date: 05/14/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02068	Calib. Date:	03/01/2016
Certification File No.:	02069	Cert. Date:	03/01/2016
Linearity File No.:	02070	Lin. Date:	03/01/2016
Solution File No.:	02114	Soln. Date:	05/14/2016
Sequential File No.:	02114	File Date:	05/14/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0341
Solution Control Lot:	201603L	Expires:	03/22/2018
		Bottle No.:	0178

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:36D		
Control 1 EC	0.000%	12:36D	34.0°C	CONTROL TEST FAILED
Control 1 IR	0.101%	12:36D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	12:37D		
Control 2 EC	0.000%	12:38D	34.0°C	CONTROL TEST FAILED
Control 2 IR	0.101%	12:38D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	12:38D		
Control 3 EC	0.000%	12:39D	34.0°C	CONTROL TEST FAILED
Control 3 IR	0.099%	12:39D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	12:39D		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____



#187

Badge No.: 187

Date: 05/14/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02117	Calib. Date: 07/19/2016
Certification File No.:	02118	Calib. No.: 00029
Linearity File No.:	02119	Cert. Date: 07/19/2016
Solution File No.:	02130	Cert. No.: 00025
Sequential File No.:	02130	Lin. Date: 07/19/2016
		Lin. No.: 00025
		Soln. Date: 08/21/2016
		Soln. No.: 00222
		File Date: 08/21/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0340
Solution Control Lot:	201605D	Expires: 05/17/2018
		Bottle No.: 0609

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	19:51D		
Control 1 EC	0.101%	19:51D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	19:51D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:52D		
Control 2 EC	0.101%	19:52D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	19:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:53D		
Control 3 EC	0.101%	19:54D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	19:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BRISTOW

First Name: MARK

MI: V

Signature: PTL. Bristow #195

Badge No.: 0195

Date: 08/21/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02117	Calib. Date:	07/19/2016
Certification File No.:	02118	Cert. No.:	00029
Linearity File No.:	02119	Cert. Date:	07/19/2016
Solution File No.:	02138	Lin. Date:	07/19/2016
Sequential File No.:	02138	Lin. No.:	00025
		Soln. Date:	09/21/2016
		Soln. No.:	00223
		File Date:	09/21/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0340
Solution Control Lot:	201605D	Expires:	05/17/2018
		Bottle No.:	1205

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:03D		
Control 1 EC	0.103%	10:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.104%	10:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:04D		
Control 2 EC	0.103%	10:05D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.102%	10:05D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:06D		
Control 3 EC	0.102%	10:06D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.103%	10:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:07D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____



Badge No.: 187

Date: 09/21/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02117	Calib. Date: 07/19/2016
Certification File No.:	02118	Calib. No.: 00029
Linearity File No.:	02119	Cert. Date: 07/19/2016
Solution File No.:	02153	Cert. No.: 00025
Sequential File No.:	02153	Lin. Date: 07/19/2016
		Lin. No.: 00025
		Soln. Date: 10/19/2016
		Soln. No.: 00224
		File Date: 10/19/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0340
Solution Control Lot:	201605D	Expires: 05/17/2018
		Bottle No.: 1204

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:09D		
Control 1 EC	0.103%	23:10D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.104%	23:10D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:10D		
Control 2 EC	0.103%	23:11D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.103%	23:11D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:12D		
Control 3 EC	0.103%	23:12D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.102%	23:12D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:13D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____

Badge No.: 187

Date: 10/19/2016

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0066
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 02117 Calib. Date: 07/19/2016 Calib. No.: 00029
Certification File No.: 02118 Cert. Date: 07/19/2016 Cert. No.: 00025
Linearity File No.: 02119 Lin. Date: 07/19/2016 Lin. No.: 00025
Solution File No.: 02161 Soln. Date: 11/19/2016 Soln. No.: 00225
Sequential File No.: 02161 File Date: 11/19/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0340
Control Solution %: 0.100% Expires: 08/04/2017
Solution Control Lot: 15H140 Bottle No.: 1190

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:11S		
Control 1 EC	0.103%	03:11S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	03:11S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:12S		
Control 2 EC	0.102%	03:12S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	03:12S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:13S		
Control 3 EC	0.102%	03:14S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	03:14S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:14S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KUCHMEK

First Name: JOSEPH

MI: -

Signature: _____

M. J. Kuchmek #2116

Badge No.: 216

Date: 11/19/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02117	Calib. Date:	07/19/2016
Certification File No.:	02118	Cert. Date:	07/19/2016
Linearity File No.:	02119	Lin. Date:	07/19/2016
Solution File No.:	02169	Soln. Date:	12/19/2016
Sequential File No.:	02169	File Date:	12/19/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0340
Solution Control Lot:	16330	Expires:	10/28/2018
		Bottle No.:	0020

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:44S		
Control 1 EC	0.103%	21:45S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	21:45S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:45S		
Control 2 EC	0.102%	21:46S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	21:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:46S		
Control 3 EC	0.102%	21:47S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	21:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:48S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____



Badge No.: 187

Date: 12/19/2016