

# Alcotest 7110 Calibration Record

## Equipment

Alcotest 7110 MKIII-C  
PENNSAUKEN TWSP. P.D.  
Serial No.: ARUM-0066


Location:			
Calibration File No.:	02340	Calib. Date: 11/27/2017	Calib. No.: 00032
Certification File No.:	02272	Cert. Date: 07/11/2017	Cert. No.: 00027
Linearity File No.:	02273	Lin. Date: 07/11/2017	Lin. No.: 00027
Solution File No.:	02333	Soln. Date: 11/15/2017	Soln. No.: 00241
Sequential File No.:	02340	File Date: 11/27/2017	

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUN S3-0341
Control Solution %:	0.100%			Expires:	10/10/2018
Solution Control Lot:	16270			Bottle No.:	1059

## Coordinator

Last Name: WATSON  
First Name: MATTHEW  
MI: R  
Signature: *Tr. II Matthew Watson* #7078  
Badge No.: 7078  
Date: 11/27/2017

\*Black Key Temperature Probe Serial.....# DDXKP2 - 390 MRW  
\*Digital NIST Temperature Measuring System Serial.....# 170428362 MPW

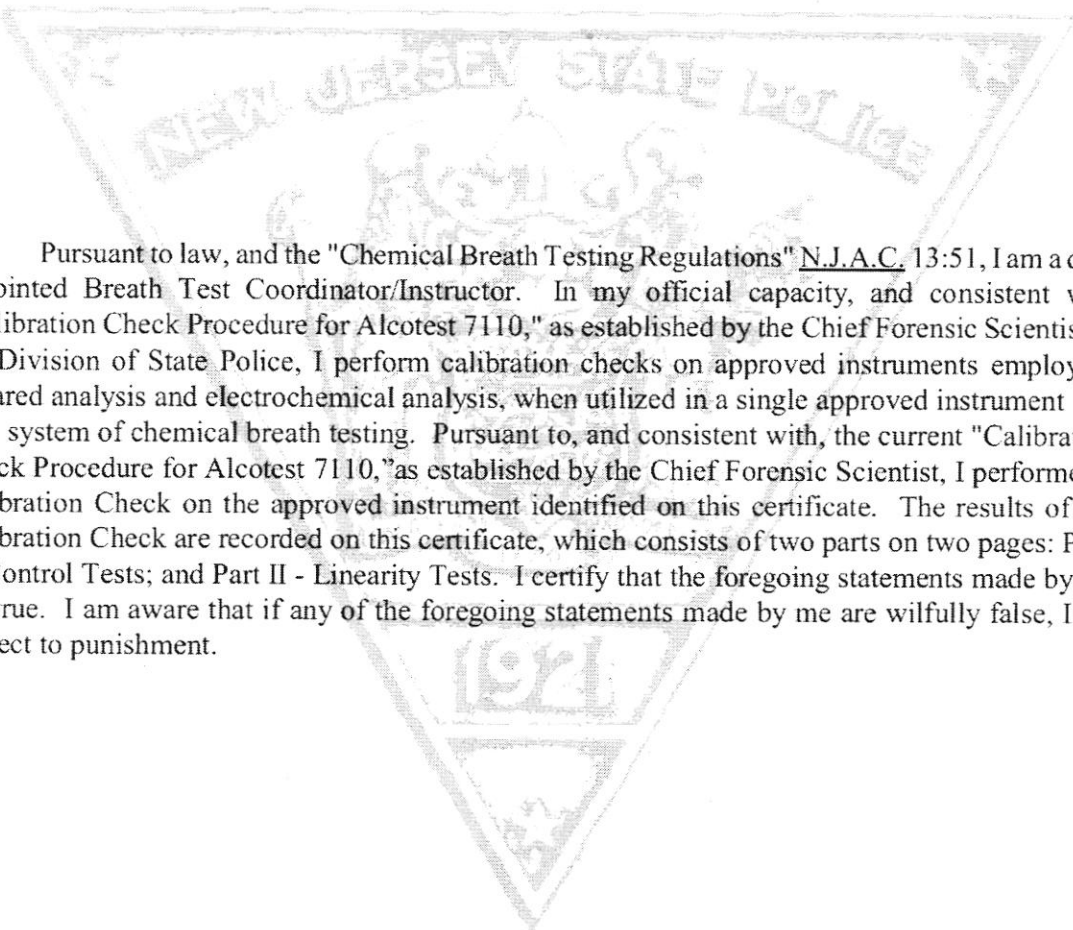

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part I - Control Tests

### Equipment

Alcotest 7110 MKIII-C  
PENNSAUKEN TWSP. P.D.  
Serial No.: ARUM-0066

Calibration File No.:	02340	Calib. Date:	11/27/2017	Calib. No.:	00032
Certification File No.:	02341	Cert. Date:	11/27/2017	Cert. No.:	00028
Linearity File No.:	02273	Lin. Date:	07/11/2017	Lin. No.:	00027
Solution File No.:	02333	Soln. Date:	11/15/2017	Soln. No.:	00241
Sequential File No.:	02341	File Date:	11/27/2017		

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUN S3-0341
Control Solution %:	0.100%			Expires:	10/10/2018
Solution Control Lot:	16270			Bottle No.:	1059

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:51S		
Control 1 EC	0.099%	08:51S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:52S		
Control 2 EC	0.098%	08:53S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:53S		
Control 3 EC	0.099%	08:54S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:55S		

All tests within acceptable tolerance.

### Coordinator

Last Name: WATSON First Name: MATTHEW MI: R

Signature: *Tpr. II Matthew A. Watson #7078* Badge No.: 7078  
Date: 11/27/2017

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.